

Angiography Catheters

Instructions for Use



T _ A N G I O 8 8 _ R E V 0

ANGIOGRAPHY CATHETERS

CAUTION: U.S. federal law restricts this device to sale by or on the order of a physician (or properly licensed practitioner).

DEVICE DESCRIPTION

Catheters for use in angiographic procedures are available in a variety of French sizes, endhole sizes, lengths, materials and designs (e.g., polyethylene or nylon, non-braided or braided with 1:1 torque).

The choice of catheter material for different angiographic procedures should be based on the physician's experience.

INTENDED USE

The catheters are intended for use in angiographic procedures by physicians trained and experienced in angiographic techniques. Standard techniques for placement of vascular access sheaths, angiographic catheters and wire guides should be employed.

CONTRAINDICATIONS

None known.

WARNINGS

None known.

PRECAUTIONS

- Manipulation of catheter requires fluoroscopic control.
- Due to thinwall construction, extreme care must be exercised during manipulation and withdrawal. Catheter insertion through a synthetic vascular graft should be avoided whenever possible.
- Do not attempt to heat or reshape the catheter curve; the catheter tip is made from a heat-sensitive material.
- The possible whiplash effect of the long, soft catheter tip must be considered during selective angiography.
- Activate hydrophilic coating, if present, by wetting the distal end of the catheter with sterile water or saline. For best results, keep the catheter surface wet during placement.
- If an over-the-wire catheter design is used, where the wire is left in place during injections, the proximal end of the wire should be clamped to protect against accidental injection of the wire guide.

INSTRUCTIONS FOR USE

The catheter has been designed for percutaneous introduction into the vascular system over an appropriately sized wire guide or through an appropriately sized sheath introducer.

Due to the catheter construction, the use of a wire guide is recommended during advancement.

If resistance is encountered during manipulation, stop and determine the cause before proceeding any further.

Peel-Away® Straightener

Catheters with pigtail shaped or similar configurations are supplied with Peel-Away straighteners to be used as follows.

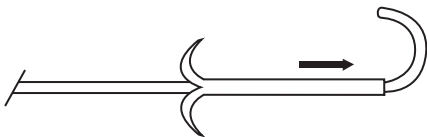


Fig. 1

1. Slide Peel-Away straightener forward to open catheter tip. (**Fig. 1**)




Fig. 2

2. With catheter tip straight, advance catheter over wire guide. (**Fig. 2**)




Fig. 3

3. After initial advancement of catheter over the wire guide, pull back and peel away the straightener for catheter introduction. (**Fig. 3**)

Peel-Away straightener must not be used as a vascular introducer sheath.

HOW SUPPLIED

Supplied sterilized by ethylene oxide gas in peel-open packages. Intended for one-time use. Sterile if package is unopened or undamaged. Do not use the product if there is doubt as to whether the product is sterile. Store in a dark, dry, cool place. Avoid extended exposure to light. Upon removal from package, inspect the product to ensure no damage has occurred.

REFERENCES

These instructions for use are based on experience from physicians and (or) their published literature. Refer to your local Cook sales representative for information on available literature.



Quantity per box



Introducer Sheath



Keep away from sunlight



Keep dry



MANUFACTURER

COOK INCORPORATED

750 Daniels Way

Bloomington, IN 47404 U.S.A.

www.cookmedical.com

© COOK 2010

October 2010